



Air Dosimetry Report



Ionizing Activity of Radon Daughter Isotopes

This report is intended to inform you of the “background radiation” in the vicinity of Kearney Nebraska.

Just as drinking water may reasonably contain radiological contaminants, dust carried in the air also contains natural radiological materials. The *Annual Water Quality Report* provided by the City of Kearney reports these values in picoCuries per liter. This report lists airborne radiological contaminants in picoCuries per cubic meter and compares the measured activity to the EPA’s benchmark for Radon in your home.

We captured dust from 16 Mar 2015 to 20 Mar 2015 ($t_{stop} \sim 95.1$ hr) in the EPA RadNet monitoring station located atop UNK’s Bruner Hall of Science. Analysis shows that during that time dust particles carrying two types of radiation emitters produced exposure in the following amounts:


$$\begin{aligned} \alpha - \text{exposure} &\approx 39.94 \text{ pCi/m}^3 \\ \beta - \text{exposure} &\approx 302.58 \text{ pCi/m}^3 \end{aligned}$$

The overall exposure rate for this time span was 342.5201 pCi/m³.

Comparing this sample to the EPA standards, the measured exposure was about 8.6% of the EPA’s benchmark for Radon in your home. The EPA recommends remediation if tests show your home contains 4000 pCi/m³ or more.

If you approximate your respiration rate to be 12 → 20 breaths per minute, and your tidal volume (the amount of air you inhale each breath) to be about 0.0005 m³/breath, then the results quoted in this report suggest an exposure in the range of (1.0789 → 1.7982)μCi/yr.

The chart below places this most recent value in context with previous results:

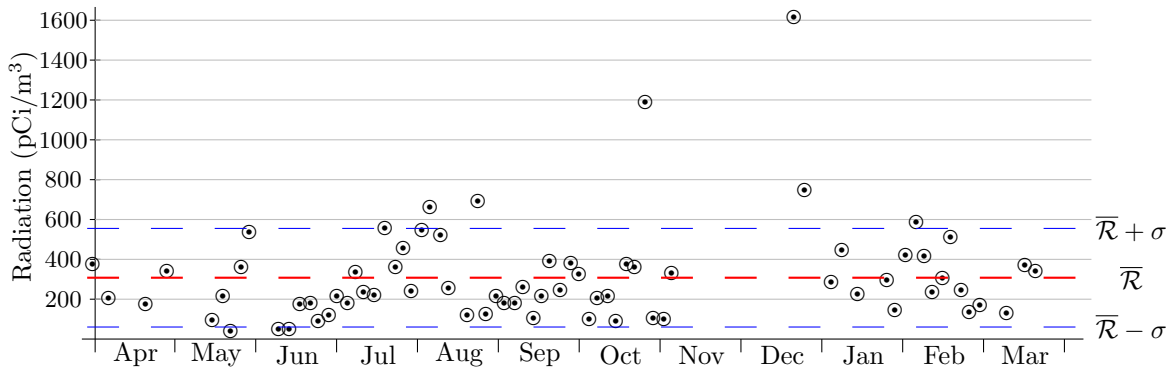

For more information regarding this and earlier reports, contact:

Robert I. Price, PhD
Department of Physics
UNK, Kearney, NE, Retired
pricerip@gmail.com
www.RipPhysics.com

Report Location: Folder # 20150320

Filter #: 425

Station #: 724 Kearney, NE

Sampled Days : 2015 03 16 → 2015 03 20

RadNet Air Monitoring

RadNet has more than 100 stationary (fixed) radiation air monitors in 48 states. . . . RadNet runs 24 hours a day, 7 days a week, and sends near-real-time measurements of beta and gamma radiation to EPA's National Air and Radiation Environmental Laboratory (NAREL). . . . Filters on the air monitors capture particles from the air (airborne particulates). Monitor operators collect the filters and send them to NAREL for testing that double-checks the monitor readings. Staff use these test results to calculate the concentration of radionuclides on the particles and find trends in airborne radiation.

The filters from each monitor are sent to EPA's NAREL, where they are analyzed for gross beta radiation. If beta activity in the sample exceeds one picocurie per cubic meter (1 pCi/m^3), the lab conducts a follow-up scan for gamma activity.

Background Radiation:

The ubiquitous ionizing radiation we are exposed to from natural as well as artificial sources in our environment is called background radiation.

Quotation from: <http://www.epa.gov/enviro/facts/radnet/>

RadNet data provides a means to estimate levels of radioactivity in the environment, including background radiation as well as radioactive fallout from atomic weapons testing, nuclear accidents, and other intrusions of radioactive materials. RadNet also provides the historical data needed to estimate long-term trends in environmental radiation levels.

Local (volunteer) monitor operators operate these EPA RadNet monitoring stations with a standardized protocol as per *NAREL Standard Operating Procedure for Using the Ludlum Alpha/Beta System for Counting RadNet Air Filters* section 6.4 Counting Air Filters: NOTE: Filters should not be counted until at least five hours after removal from the air sampler, to allow time for decay of interfering radon daughter isotopes.

For More Information: www.epa.gov/radnet/index.html

UNK's Auxiliary Protocol

This report is the result of a protocol developed at UNK to determine the activity of the interfering radon daughter isotopes highlighted in section 6.4 of the NAREL defined protocol. With this we develop a near real-time exposure history to short lived isotopes carried by airborne dust in our local area. As the air sampler is switched off the radiation load on the filter begins to diminish exponentially.

$$\mathcal{A} = \mathcal{A}_1 e^{-\lambda_1 t} + \mathcal{A}_2 e^{-\lambda_2 t}$$

Measuring the "decay" curves for the Alpha and Beta emitters we determine the accumulated activity for each at the moment the sampler was turned off ($t = t_{\text{stop}}$). We then estimate the accumulation rate (\mathcal{R}) for each type of ionizing radiation (α and β) trapped in the filter as the sampler ran for 3 or 4 days ($\approx 72 \text{ hr}$ or $\approx 94 \text{ hr}$).

$$\mathcal{R} = \left\{ \frac{\lambda_1 \mathcal{A}_1}{(1 - e^{-\lambda_1 t})} + \frac{\lambda_2 \mathcal{A}_2}{(1 - e^{-\lambda_2 t})} \right\} \Big|_{t=t_{\text{stop}}}$$

While the rate of deposition is most likely not constant, we can estimate the average rate of deposition over the hours of sampling time, and use it to determine an approximate concentration in the air.

Data on the next two pages illustrate how the reported result is calculated.

α Data

Table 1: Alpha Activity

Time (hr)	Count Rate (pCi)
0.15	2970.24
0.33333	2563.68
0.5	2476.32
0.75	2078.16
1	1846.32
1.33333	1732.08
1.83333	1380.96
2.66667	1249.92
3.91667	1196.16
5.86667	986.16
10	794.64

The best fit to the data suggests two time constants for the Alpha particle emitters with their associated activities at the moment the sampler was shutdown.

$$\mathcal{A}_1 = 1909.4 \text{ pCi} \quad \lambda_1 = 1.215 \text{ hr}^{-1} \quad \mathcal{A}_2 = 1383 \text{ pCi} \quad \lambda_2 = 0.054868 \text{ hr}^{-1}$$

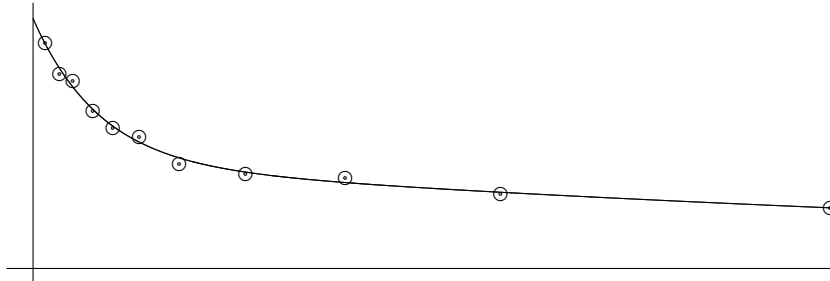


Figure 1: α Activity versus Time

This sketch¹ exists only to provide a visual representation of the phenomenological fit to the data.

α emitting radon daughter isotopes arrived at the filter with an average rate given by:

$$\mathcal{R} = \frac{\lambda \mathcal{A}_{\text{stop}}}{(1 - e^{-\lambda t_{\text{stop}}})} \Rightarrow \mathcal{R}_1 = 2319.9210 \frac{\text{pCi}}{\text{hr}} @ \tau_1 = 0.82 \text{ hr} , \text{ and } , \mathcal{R}_2 = 76.2962 \frac{\text{pCi}}{\text{hr}} @ \tau_2 = 18.23 \text{ hr}$$

$$\mathcal{R} \times 95.083333 \text{ hr} / 5704.9 \text{ m}^3 \approx 38.6660 \text{ pCi/m}^3, \text{ and } , 1.2716 \text{ pCi/m}^3.$$

Report Location: Folder # 20150320

Filter #: 425

Station #: 724 Kearney, NE

Sampled Days : 2015 03 16 → 2015 03 20

¹The axes have neither scales nor units.

β Data

Table 2: Beta Activity

Time (hr)	Count Rate (pCi)
0.15	22445.39
0.33333	20607.13
0.5	18565.57
0.75	16091.73
1	14753.16
1.33333	12536.12
1.83333	11419.04
2.66667	9887.87
3.91667	8840.34
5.86667	7882.69
10	5617.5

The best fit to the data suggests two time constants for the Beta particle emitters with their associated activities at the moment the sampler was shutdown.

$$\mathcal{A}_1 = 13988 \text{ pCi} \quad \lambda_1 = 1.2442 \text{ hr}^{-1} \quad \mathcal{A}_2 = 11257 \text{ pCi} \quad \lambda_2 = 0.066574 \text{ hr}^{-1}$$

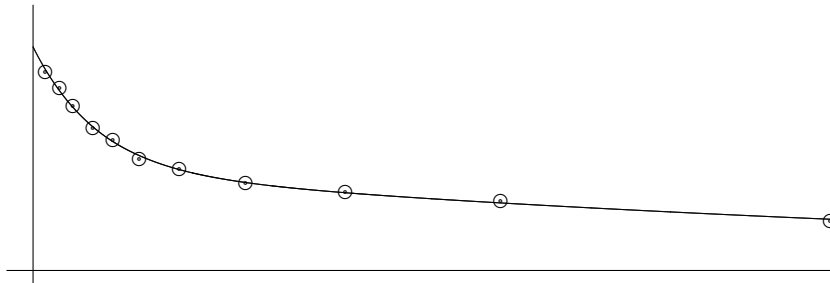


Figure 2: β Activity versus Time

This sketch² exists only to provide a visual representation of the phenomenological fit to the data.

β emitting radon daughter isotopes arrived at the filter with an average rate given by:

$$\mathcal{R} = \frac{\lambda \mathcal{A}_{\text{stop}}}{(1 - e^{-\lambda t_{\text{stop}}})} \Rightarrow \mathcal{R}_1 = 17403.8696 \frac{\text{pCi}}{\text{hr}} @ \tau_1 = 0.80 \text{ hr} , \text{ and } , \mathcal{R}_2 = 750.7613 \frac{\text{pCi}}{\text{hr}} @ \tau_2 = 15.02 \text{ hr}$$

$$\mathcal{R} \times 95.083333 \text{ hr} / 5704.9 \text{ m}^3 \approx 290.0696 \text{ pCi/m}^3, \text{ and } , 12.5129 \text{ pCi/m}^3.$$

Report Location: Folder # 20150320

Filter #: 425

Station #: 724 Kearney, NE

Sampled Days : 2015 03 16 \rightarrow 2015 03 20

²The axes have neither scales nor units.